


10 Documents joints

- Schéma de pièces de rechange et de montage : 42/018-Z03-01-2
- Déclaration de conformité : KX420009
- Attestations : FM16NCA0008, FM16NUS0017
- RMA - Déclaration de décontamination

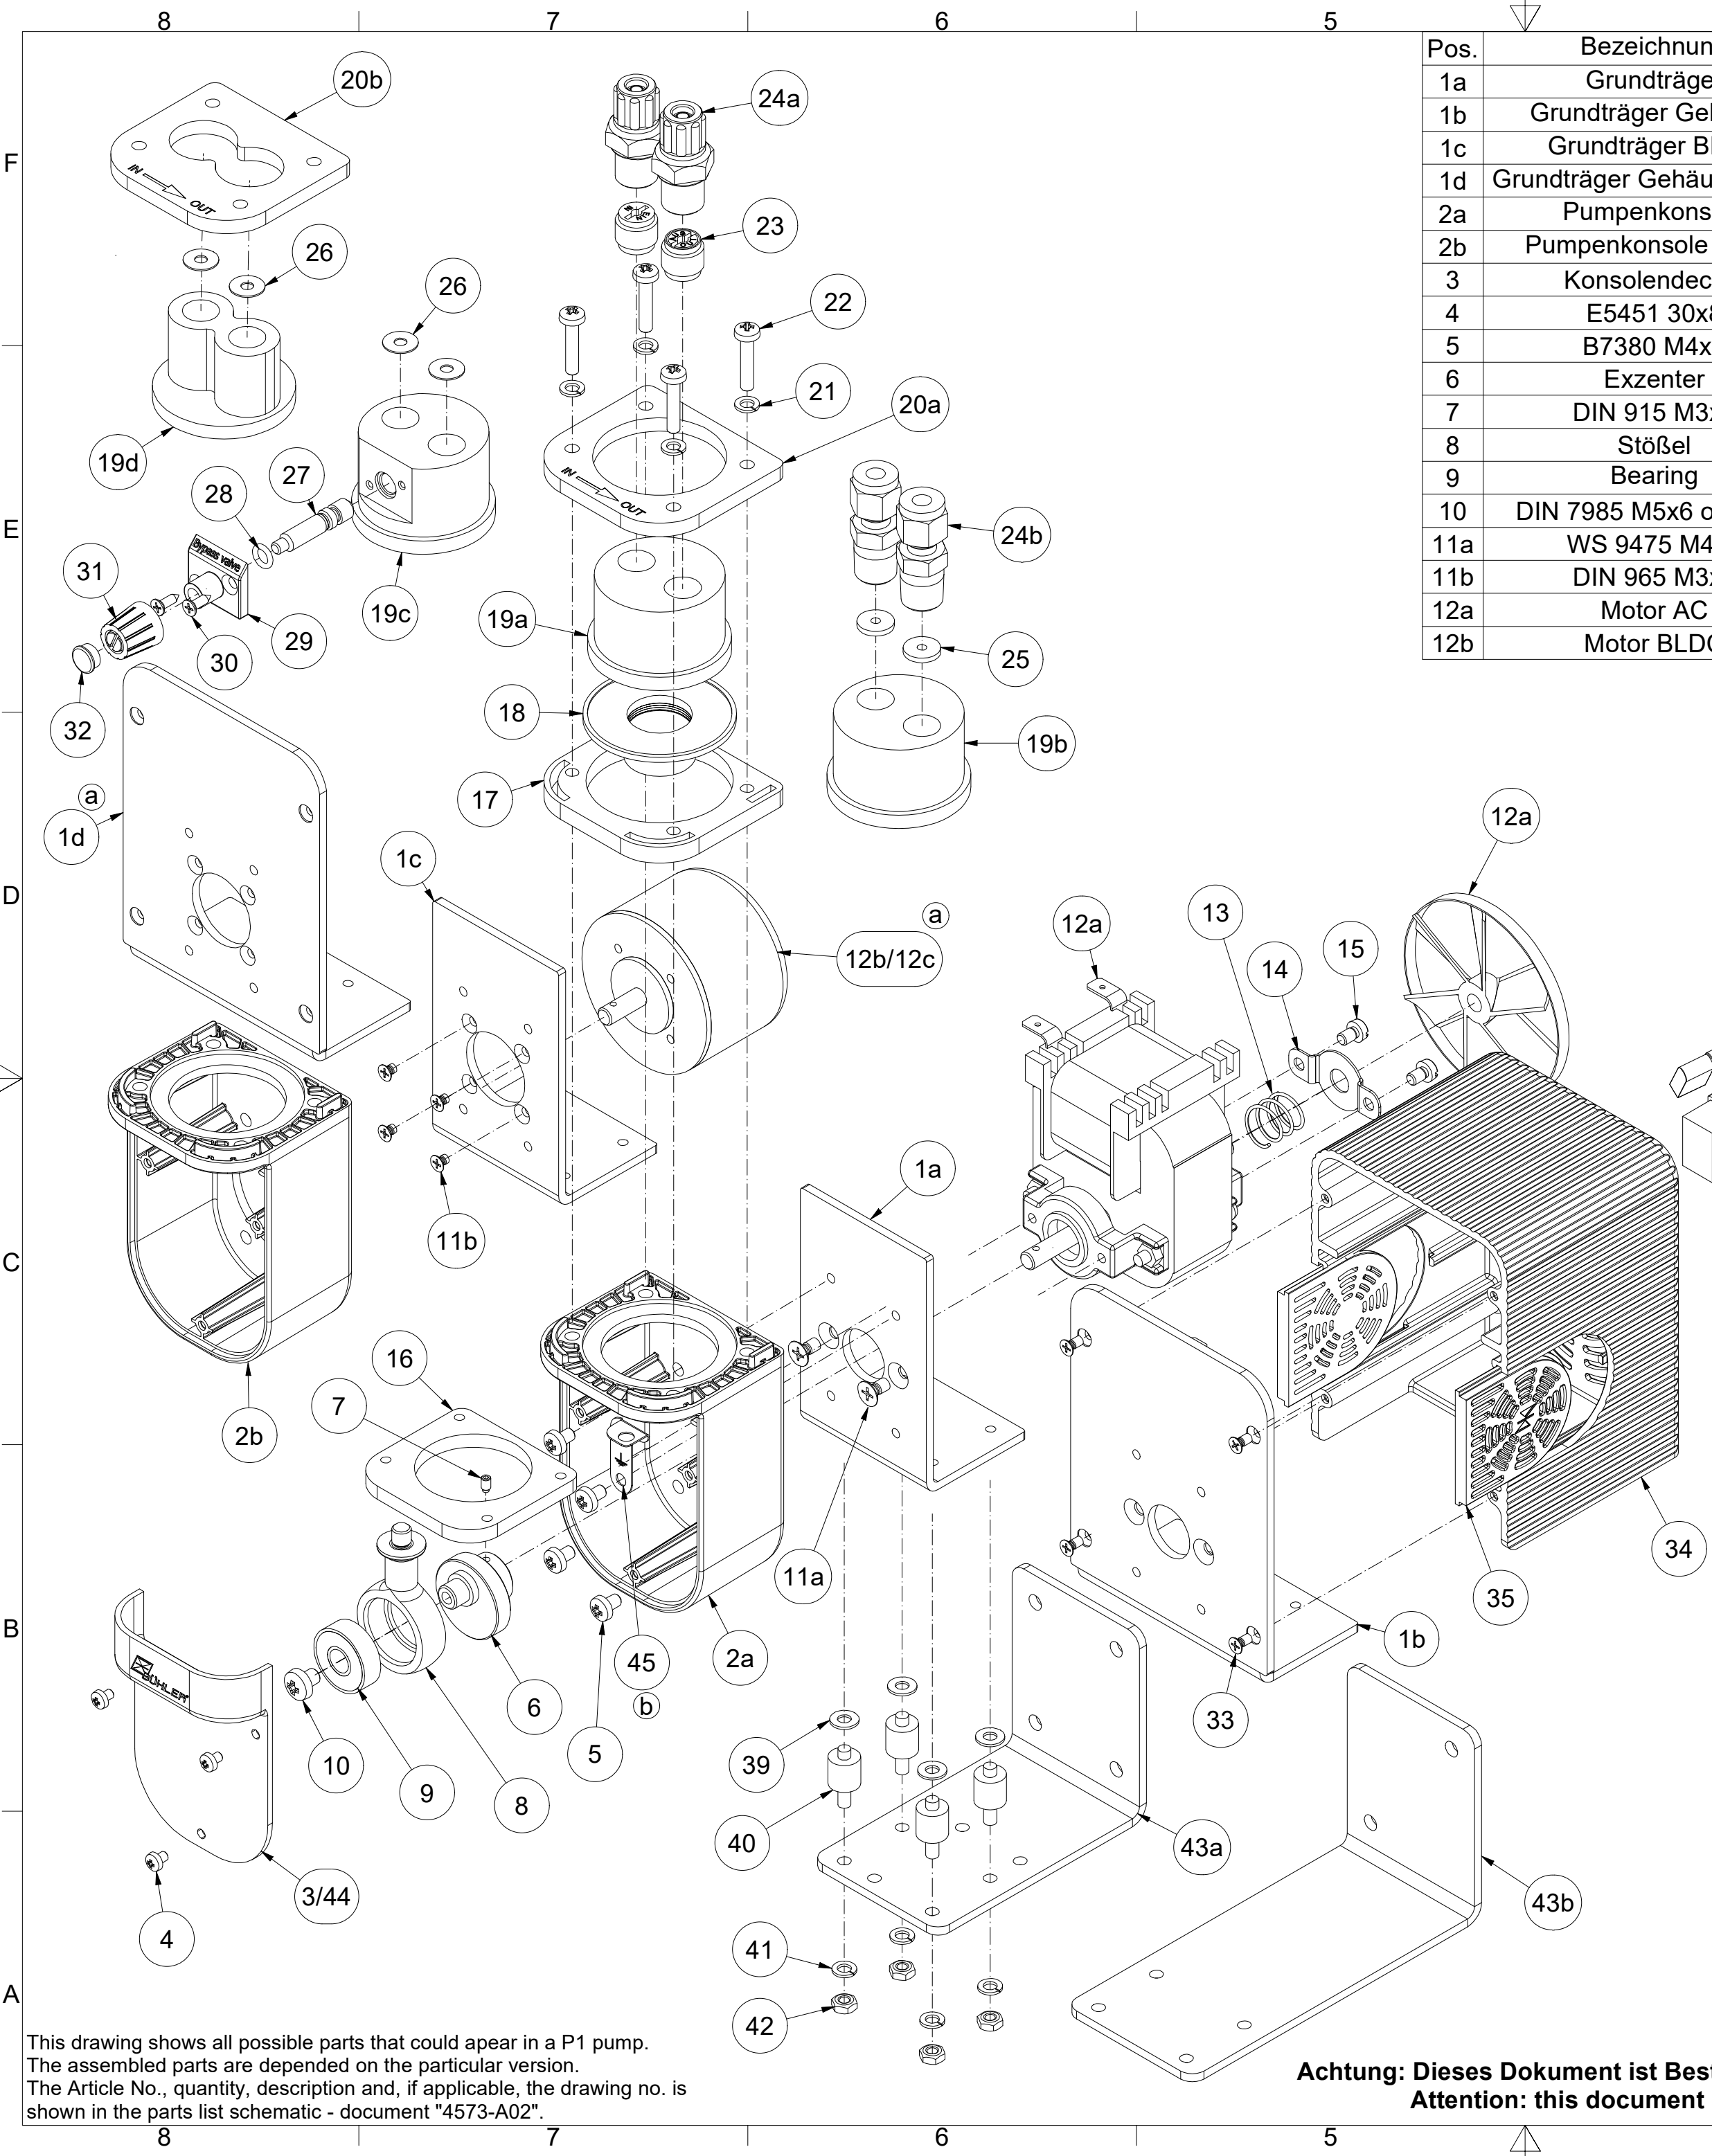

Pos.	Bezeichnung	Description	Pos.	Bezeichnung	Description
1a	Grundträger	base angel	12c	Motor BLDC mit Stecker	motor bldc with plug
1b	Grundträger Gehäuse	base angel enclosure	13	Feder	spring
1c	Grundträger BLDC	base angel bldc	14	Erdungsblech	protective ground sheet
1d	Grundträger Gehäuse BLDC	base angel enclosure bldc	15	DIN 85 M4x6	DIN 85 M4x6
2a	Pumpenkonsole	pump console	16	Gegenring	counter ring
2b	Pumpenkonsole BLDC	pump console bldc	17	Abdeckung	cover
3	Konsolendeckel	cover	18	Faltenbalg	bellow
4	E5451 30x8	E5451 30x8	19a	Pumpenkörper PTFE	pump head PTFE
5	B7380 M4x6	B7380 M4x6	19b	Pumpenkörper VA	pump head SS
6	Exzenter	Eccentric	19c	Pumpenkörper PVDF Bypass	pump head PVDF bypass
7	DIN 915 M3x5	DIN 915 M3x5	19d	Pumpenkörper PVDF	pump head PVDF
8	Stößel	Plunger	20a	Befestigungsring	mounting ring
9	Bearing	Kugellager	20b	Befestigungsring nur PVDF Körper	mounting ring only PVDF head
10	DIN 7985 M5x6 or M5x8	DIN 7985 M5x6 or M5x8	21	DIN 127 B4,1 oder DIN 6796	DIN 127 B4,1 or DIN 6796
11a	WS 9475 M4x8	WS 9475 M4x8	22	B7380 M4x20	B7380 M4x20
11b	DIN 965 M3x6	DIN 965 M3x6	23	Ein- Auslassventil	In- Outletvalve
12a	Motor AC	motor AC	24a	Verschraubung PVDF	Fitting PVDF
12b	Motor BLDC	motor bldc	24b	Verschraubung VA	Fitting SS

Pos.	Bezeichnung	Description	Pos.	Bezeichnung	Description
12c	Motor BLDC mit Stecker	motor bldc with plug	19a	Pumpenkörper PTFE	pump head PTFE
13	Feder	spring	19b	Pumpenkörper VA	pump head SS
14	Erdungsblech	protective ground sheet	19c	Pumpenkörper PVDF Bypass	pump head PVDF bypass
15	DIN 85 M4x6	DIN 85 M4x6	19d	Pumpenkörper PVDF	pump head PVDF
16	Gegenring	counter ring	20a	Befestigungsring	mounting ring
17	Abdeckung	cover	20b	Befestigungsring nur PVDF Körper	mounting ring only PVDF head
18	Faltenbalg	bellow	21	DIN 127 B4,1 oder DIN 6796	DIN 127 B4,1 or DIN 6796
19a	Pumpenkörper PTFE	pump head PTFE	22	B7380 M4x20	B7380 M4x20
19b	Pumpenkörper VA	pump head SS	23	Ein- Auslassventil	In- Outletvalve
19c	Pumpenkörper PVDF Bypass	pump head PVDF bypass	24a	Verschraubung PVDF	Fitting PVDF
19d	Pumpenkörper PVDF	pump head PVDF	24b	Verschraubung VA	Fitting SS
20a	Befestigungsring	mounting ring	25	Verdränger	displacer
20b	Befestigungsring nur PVDF Körper	mounting ring only PVDF head	26	Dichtscheibe	valve sealing
21	DIN 127 B4,1 oder DIN 6796	DIN 127 B4,1 or DIN 6796	27	Spindel	spindle
22	B7380 M4x20	B7380 M4x20	28	O-Ring	o-ring
23	Ein- Auslassventil	In- Outletvalve	29	Ventilplatte	valve plate
24a	Verschraubung PVDF	Fitting PVDF	30	DIN 7982 2,9x9,5	DIN 7982 2,9x9,5
24b	Verschraubung VA	Fitting SS	31	Drehknopf	knob
25	Verdränger	displacer	32	Abdeckung	cover
26	Dichtscheibe	valve sealing	33	E5454 30x8	E5454 30x8
27	Spindel	spindle	34	Gehäuseteil 1	enclosure part 1
28	O-Ring	o-ring	35	Gehäuseteil 2	enclosure part 2
29	Ventilplatte	valve plate	36	Kabelverschraubung	cable gland
30	DIN 7982 2,9x9,5	DIN 7982 2,9x9,5	37	Blindstopfen	dummy plug
31	Drehknopf	knob	38	Anschlusskabel	connection cable
32	Abdeckung	cover	38a	Anschlusskabel BLDC	connection cable bldc
33	E5454 30x8	E5454 30x8	39	DIN 125 A4,3	DIN 125 A4,3
34	Gehäuseteil 1	enclosure part 1	40	Gummi Puffer	vibration damper
35	Gehäuseteil 2	enclosure part 2	41	DIN 127 B4,1 oder DIN 6796	DIN 127 B4,1 or DIN 6796
36	Kabelverschraubung	cable gland	42	DIN 934 M4	DIN 934 M4
37	Blindstopfen	dummy plug	43a	Montagekonsole	Mounting console
38	Anschlusskabel	connection cable	43b	Montagekonsole Gehäuse	Mounting console enclosure
38a	Anschlusskabel BLDC	connection cable bldc	44	Konsolendeckel mit Lüftungsschlitzen	Cover with ventilation slots
39	DIN 125 A4,3	DIN 125 A4,3	45	Potentialausgleichsblech	Equipotential bonding sheet
40	Gummi Puffer	vibration damper			
41	DIN 127 B4,1 oder DIN 6796	DIN 127 B4,1 or DIN 6796			
42	DIN 934 M4	DIN 934 M4			
43a	Montagekonsole	Mounting console			
43b	Montagekonsole Gehäuse	Mounting console enclosure			
44	Konsolendeckel mit Lüftungsschlitzen	Cover with ventilation slots			
45	Potentialausgleichsblech	Equipotential bonding sheet			

Ersatzteile / Spare parts			
Bezeichnung	Description	Artikel Nr. / Article no.	Pos.Nr. / Pos. no.
Kurbeltrieb	crank assembly	4228065	6/7/8/9/10
Faltenbalg	bellow	4228003	18
Ventil 70°C (1 Stück)	Valve 70°C (1 piece)	4228006	23
Ventil 70°C (2 Stück)	Valve 70°C (2 Stück)	4228066	23/26
O-Ring	O-ring	9009398	28
Montagekonsole	Mounting console	4228060	43a
Montagekonsole Gehäuse	Mounting console enclosure	4228067	43b
Pufferset	Damper set	4228061	39/40/41/42
Montagekonsole & Pufferset	Mounting console & damper set	4228062	39/40/41/42/43a
Montagekonsole & Pufferset	Mounting console & damper set	4228063	39/40/41/42/43b

This drawing shows all possible parts that could appear in a P1 pump.
The assembled parts are depended on the particular version.
The Article No., quantity, description and, if applicable, the drawing no. is shown in the parts list schematic - document "4573-A02".

Achtung: Dieses Dokument ist Bestandteil der FM-Zulassung
Attention: this document is part of the FM-Approval

Alle Kanten gratfrei	Alle Rechte vorbehalten	Maße ohne Toleranzangabe nach ISO 2768-mK	Maßstab: 1:1,6	Masse:
✓ = √ R0		Datum: 13.10.2015	Werkstoff:	
✓/ = √ Rz 63		Name: Sundergeld	Benennung: Exploded view of the P1.x Pumps	
✓ = √ Rz 16		Bearb. 24.10.19	ZeichnungsNr.: 42/018-Z03-01-2B	
✓ = √ Rz 4		Gepr.	Art.Nr.: 42...	
			Arbeitsanweisung:	

EG-/EU Konformitätserklärung
EC/EU Declaration of Conformity



Hiermit erklärt Bühler Technologies GmbH,
dass die nachfolgenden Produkte den
wesentlichen Anforderungen der Richtlinie

2006/42/EG
(MRL)

in ihrer aktuellen Fassung entsprechen.

Die Produkte sind Maschinen nach Artikel 2 a).

*Herewith declares Bühler Technologies GmbH
that the following products correspond to the
essential requirements of Directive*

2006/42/EC
(MD)

in its actual version.

*The products are machines according to
article 2 (a).*

Produkt / products: Messgaspumpe / Sample gas pump
Typ / type: P 1.x

Das Betriebsmittel ist für den Einbau in Gasanalysesystemen bestimmt und für das Fördern von
ausschließlich gasförmigen Medien vorgesehen.

*The equipment is designed for installation in gas analyser systems and is designed to transport only
gaseous media.*

Das oben beschriebene Produkt der Erklärung erfüllt die einschlägigen
Harmonisierungsrechtsvorschriften der Union:

*The object of the declaration described above is in conformity with the relevant Union harmonisation
legislation:*

EN 809:1998+A1:2009 + AC:2010

EN 60204-1:2018

Zusätzlich wurden berücksichtigt:
In addition, the following standards have been used:
EN ISO 12100:2010

Die alleinige Verantwortung für die Ausstellung dieser Konformitätserklärung trägt der Hersteller.
This declaration of conformity is issued under the sole responsibility of the manufacturer.

Dokumentationsverantwortlicher für diese Konformitätserklärung ist Herr Stefan Eschweiler mit
Anschrift am Firmensitz.

*The person authorised to compile the technical file is Mr. Stefan Eschweiler located at the company's
address.*

Ratingen, den 15.09.2022

Stefan Eschweiler
Geschäftsführer – Managing Director

Frank Pospiech
Geschäftsführer – Managing Director

UK Declaration of Conformity



The manufacturer Bühler Technologies GmbH declares, under the sole responsibility, that the product complies with the requirements of the following UK legislation:

Machinery Safety Regulations 2008

Product: Sample gas pump

Type: P 1.x

The equipment is designed for installation in gas analyser systems and is designed to transport only gaseous media.

The object of the declaration described above is in conformity with the relevant designated standards:

EN 809:1998+A1:2009 + AC:2010

EN 60204-1:2018

In addition, the following standards have been used:

EN ISO 12100:2010

Ratingen in Germany, 01.11.2022

A handwritten signature in blue ink, appearing to read 'Stefan Eschweiler', written over a horizontal line.

Stefan Eschweiler
Managing Director

A handwritten signature in blue ink, appearing to read 'Frank Pospiech', written over a horizontal line.

Frank Pospiech
Managing Director



Member of the FM Global Group

FM Approvals
1151 Boston Providence Turnpike
P.O. Box 9102 Norwood, MA 02062 USA
T: 781 762 4300 F: 781-762-9375 www.fmapprovals.com

CERTIFICATE OF COMPLIANCE

ELECTRICAL EQUIPMENT PER CANADIAN REQUIREMENTS

This certificate is issued for the following equipment:

4228abc1def00FM. P1.1 Sample Gas Pump.

a = Motor voltage: 1, 2, 3 or 4.
b = Pump head position: 1 or 2.
c = Pump head material: 1, 2, 3 or 4.
d = Screw-in connections / pipe fitting: 0, 1, 2, 3, 5 or 6.
e = Mounting accessories: 0, 1 or 2.
f = Housing: 0, 1 or 2.

Equipment Ratings:

Electrical Equipment for use indoor unclassified or Ordinary locations.

FM Approved for:

Bühler Technologies GmbH
Ratingen, Germany

To verify the availability of the Approved product, please refer to www.approvalguide.com

This certifies that the equipment described has been found to comply with the following Approval Standards and other documents:

CAN C22.2 No. 213	2012
CAN C22.2 No. 1010.1	2004

Original Project ID: 3057155CGP

Approval Granted: April 11, 2016

Subsequent Revision Reports / Date Approval Amended

Report Number	Date	Report Number	Date
---------------	------	---------------	------

FM Approvals LLC



J.E. Marquedant
Manager, Electrical Systems

11 April 2016

Date

To verify the availability of the Approved product, please refer to www.approvalguide.com

CERTIFICATE OF CONFORMITY



1. **ELECTRICAL EQUIPMENT PER CANADIAN REQUIREMENTS**

2. **Certificate No:** FM16NCA0008

3. **Equipment:** P1.1 Sample Gas Pumps
(Type Reference and Name)

4. **Name of Listing Company:** Bühler Technologies GmbH

5. **Address of Listing Company:** Harkortstraße 29
40880, Ratingen, Germany

6. The examination and test results are recorded in confidential report number:

3057155 dated 11th April 2016

7. FM Approvals LLC, certifies that the equipment described has been found to comply with the following Approval standards and other documents:

CSA-C22.2 No. 213:2012, CAN/CSA-C22.2 No. 61010-1:2004

8. This certificate relates to the design, examination and testing of the products specified herein. The FM Approvals surveillance audit program has further determined that the manufacturing processes and quality control procedures in place are satisfactory to manufacture the product as examined, tested and Approved.

9. **Equipment Ratings:**

Electrical equipment for use indoor unclassified or Ordinary locations

Certificate issued by:

J. E. Marquedant
Manager, Electrical Systems

9 December 2016

Date

To verify the availability of the Approved product, please refer to www.approvalguide.com

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC, 1151 Boston-Providence Turnpike, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmapprovals.com www.fmapprovals.com

SCHEDULE



to Canadian Certificate Of Conformity No: FM16NCA0008

10. Description of Equipment:

The P1 sample gas pumps carry gases from various processes to analyzers. The gas circuit typically has additional analysis components such as sample gas probe, filter, flow meter, cooler, etc. The sample gas pump P1 consists of the main components, the pump head and motor. An eccentric converts the rotation of the motor into an up and down motion using a connecting rod, thus producing the pump mechanism. Inside the so-called pump body, above the bellows, which facilitates the pump motion, are inlet and outlet valves. The user connects the gas circuits to the sample gas pump through screw-in connections.

The P1 sample gas pumps are available as 12Vdc, 24Vdc, 115Vac, 60Hz or 230Vac, 50Hz. The 115Vac and 230Vac sample gas pumps are available with or without a cover over the electronics and motor. The 115Vac and 230Vac sample gas pumps have internal self resetting thermal protection built into the motor. The P1.1 sample gas pump is for general purpose non-hazardous locations.

Model Code Structure:

4228abc1def00FM. P1.1 Sample Gas Pump.

a = Motor voltage: 1, 2, 3 or 4.

b = Pump head position: 1 or 2.

c = Pump head material: 1, 2, 3 or 4.

d = Screw-in connections / pipe fitting: 0, 1, 2, 3, 5 or 6.

e = Mounting accessories: 0, 1 or 2.

f = Housing: 0 or 1

11. Test and Assessment Procedure and Conditions:

This Certificate has been issued in accordance with FM Approvals Canadian Certification Requirements.

12. Schedule Drawings

A copy of the technical documentation has been kept by FM Approvals.

13. Certificate History

Details of the supplements to this certificate are described below:

Date	Description
11 th April 2016	Original Issue.
9 th December 2016	<u>Supplement 1:</u> Report Reference: – RR207245 dated 9 th December 2016 Description of the Change: Changes per this revision request are for the NI version of the product and don't affect this certificate. This certificate has been put into the new format.

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC. 1151 Boston-Providence Turnpike, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmaprovals.com www.fmaprovals.com

CERTIFICATE OF CONFORMITY



1. **ELECTRICAL EQUIPMENT PER CANADIAN REQUIREMENTS**

2. **Certificate No:** FM16NCA0008

3. **Equipment:** P1.1 Sample Gas Pumps
(Type Reference and Name)

4. **Name of Listing Company:** Bühler Technologies GmbH

5. **Address of Listing Company:** Harkortstraße 29
40880, Ratingen, Germany

6. The examination and test results are recorded in confidential report number:

3057155 dated 11th April 2016

7. FM Approvals LLC, certifies that the equipment described has been found to comply with the following Approval standards and other documents:

CSA-C22.2 No. 213:2012, CAN/CSA-C22.2 No. 61010-1:2004

8. This certificate relates to the design, examination and testing of the products specified herein. The FM Approvals surveillance audit program has further determined that the manufacturing processes and quality control procedures in place are satisfactory to manufacture the product as examined, tested and Approved.

9. **Equipment Ratings:**

Electrical equipment for use indoor unclassified or Ordinary locations

Certificate issued by:

J.E. Marquedant
VP, Manager - Electrical Systems

2 April 2020

Date

To verify the availability of the Approved product, please refer to www.approvalguide.com

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC, 1151 Boston-Providence Turnpike, Norwood, MA 02062 USA
T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmaprovals.com www.fmaprovals.com

SCHEDULE



to Canadian Certificate Of Conformity No: FM16NCA0008

10. Description of Equipment:

The P1 sample gas pumps carry gases from various processes to analyzers. The gas circuit typically has additional analysis components such as sample gas probe, filter, flow meter, cooler, etc. The sample gas pump P1 consists of the main components, the pump head and motor. An eccentric converts the rotation of the motor into an up and down motion using a connecting rod, thus producing the pump mechanism. Inside the so-called pump body, above the bellows, which facilitates the pump motion, are inlet and outlet valves. The user connects the gas circuits to the sample gas pump through screw-in connections.

The P1 sample gas pumps are available as 12Vdc, 24Vdc, 115Vac, 60Hz or 230Vac, 50Hz. The 115Vac and 230Vac sample gas pumps have internal self resetting thermal protection built into the motor. The P1.1 sample gas pump is for general purpose non-hazardous locations.

Model Code Structure:

4228abc1def00FM. P1.1 Sample Gas Pump.

a = Motor voltage: 1, 2, 3 or 4.

b = Pump head position: 1 or 2.

c = Pump head material: 1, 2, 3 or 4.

d = Screw-in connections / pipe fitting: 0, 1, 2, 3, 5 or 6.

e = Mounting accessories: 0, 1 or 2.

f = Housing: 0 or 1

11. Test and Assessment Procedure and Conditions:

This Certificate has been issued in accordance with FM Approvals Canadian Certification Requirements.

12. Schedule Drawings

A copy of the technical documentation has been kept by FM Approvals.

13. Certificate History

Details of the supplements to this certificate are described below:

Date	Description
11 th April 2016	Original Issue.
9 th December 2016	<u>Supplement 1:</u> Report Reference: – RR207245 dated 9 th December 2016. Description of the Change: Changes per this revision request are for the NI version of the product and don't affect this certificate. This certificate has been put into the new format.
2 nd April 2020	<u>Supplement 2:</u> Report Reference: – PR455937 dated 2 nd April 2020.

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC. 1151 Boston-Providence Turnpike, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmaprovals.com www.fmaprovals.com

SCHEDULE



to Canadian Certificate Of Conformity No: FM16NCA0008

Date	Description
	Description of the Change: Add option for gas pump cover DC motors.

FM Approvals

FM Approvals

FM Approvals

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC. 1151 Boston-Providence Turnpike, Norwood, MA 02062 USA
T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmaprovals.com www.fmaprovals.com



Member of the FM Global Group

FM Approvals
1151 Boston Providence Turnpike
P.O. Box 9102 Norwood, MA 02062 USA
T: 781 762 4300 F: 781-762-9375 www.fmapprovals.com

CERTIFICATE OF COMPLIANCE

ELECTRICAL EQUIPMENT

This certificate is issued for the following equipment:

4228abc1def00FM. P1.1 Sample Gas Pump.

a = Motor Voltage: 1, 2, 3 or 4.
b = Pump head position: 1 or 2.
c = Pump head material: 1, 2, 3 or 4.
d = Screw-in connections / pipe fitting: 0, 1, 2, 3, 5 or 6.
e = Mounting accessories: 0, 1 or 2.
f = Housing: 0, 1 or 2.

Equipment Ratings:

Electrical Equipment for use indoor unclassified or Ordinary locations.

FM Approved for:

Bühler Technologies GmbH
Ratingen, Germany

To verify the availability of the Approved product, please refer to www.approvalguide.com

This certifies that the equipment described has been found to comply with the following Approval Standards and other documents:

FM3810

2005

Original Project ID: 3057155GP


Approval Granted: April 11, 2016

Subsequent Revision Reports / Date Approval Amended

Report Number Date

Report Number Date

FM Approvals LLC



J.E. Marquedant
Manager, Electrical Systems

11 April 2016

Date

To verify the availability of the Approved product, please refer to www.approvalguide.com

CERTIFICATE OF CONFORMITY



1. **ELECTRICAL EQUIPMENT PER US REQUIREMENTS**

2. **Certificate No:** FM16NUS0017

3. **Equipment:** P1.1 Sample Gas Pumps
(Type Reference and Name)

4. **Name of Listing Company:** Bühler Technologies GmbH

5. **Address of Listing Company:** Harkortstraße 29
40880, Ratingen, Germany

6. The examination and test results are recorded in confidential report number:

3057155 dated 11th April 2016

7. FM Approvals LLC, certifies that the equipment described has been found to comply with the following Approval standards and other documents:

FM Class 3810:2005

8. This certificate relates to the design, examination and testing of the products specified herein. The FM Approvals surveillance audit program has further determined that the manufacturing processes and quality control procedures in place are satisfactory to manufacture the product as examined, tested and Approved.

9. **Equipment Ratings:**

Electrical equipment for use indoor unclassified or Ordinary locations.

Certificate issued by:

J.E. Marquedant
Manager, Electrical Systems

9 December 2016

Date

To verify the availability of the Approved product, please refer to www.approvalguide.com

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC, 1151 Boston-Providence Turnpike, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmapprovals.com www.fmapprovals.com

SCHEDULE

to US Certificate Of Conformity No: FM16NUS0017

10. Description of Equipment:

The P1 sample gas pumps carry gases from various processes to analyzers. The gas circuit typically has additional analysis components such as sample gas probe, filter, flow meter, cooler, etc. The sample gas pump P1 consists of the main components, the pump head and motor. An eccentric converts the rotation of the motor into an up and down motion using a connecting rod, thus producing the pump mechanism. Inside the so-called pump body, above the bellows, which facilitates the pump motion, are inlet and outlet valves. The user connects the gas circuits to the sample gas pump through screw-in connections.

The P1 sample gas pumps are available as 12Vdc, 24Vdc, 115Vac, 60Hz or 230Vac, 50Hz. The 115Vac and 230Vac sample gas pumps are available with or without a cover over the electronics and motor. The 115Vac and 230Vac sample gas pumps have internal self resetting thermal protection built into the motor. The P1.1 sample gas pump is for general purpose non-hazardous locations.

Model Code Structure:

4228abc1def00FM. P1.1 Sample Gas Pump.

a = Motor voltage: 1, 2, 3 or 4.

b = Pump head position: 1 or 2.

c = Pump head material: 1, 2, 3 or 4.

d = Screw-in connections / pipe fitting: 0, 1, 2, 3, 5 or 6.

e = Mounting accessories: 0, 1 or 2.

f = Housing: 0 or 1

11. Test and Assessment Procedure and Conditions:

This Certificate has been issued in accordance with FM Approvals US Certification Requirements.

12. Schedule Drawings

A copy of the technical documentation has been kept by FM Approvals.

13. Certificate History

Details of the supplements to this certificate are described below:

Date	Description
11 th April 2016	Original Issue.
9 th December 2016	<u>Supplement 1:</u> Report Reference: – RR207245 dated 9 th December 2016 Description of the Change: Changes per this revision request are for the NI version of the product and don't affect this certificate. This certificate has been put into the new format.

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

CERTIFICATE OF CONFORMITY



1. **ELECTRICAL EQUIPMENT PER US REQUIREMENTS**

2. **Certificate No:** FM16NUS0017

3. **Equipment:** P1.1 Sample Gas Pumps
(Type Reference and Name)

4. **Name of Listing Company:** Bühler Technologies GmbH

5. **Address of Listing Company:** Harkortstraße 29
40880, Ratingen, Germany

6. The examination and test results are recorded in confidential report number:

3057155 dated 11th April 2016

7. FM Approvals LLC, certifies that the equipment described has been found to comply with the following Approval standards and other documents:

FM Class 3810:2005

8. This certificate relates to the design, examination and testing of the products specified herein. The FM Approvals surveillance audit program has further determined that the manufacturing processes and quality control procedures in place are satisfactory to manufacture the product as examined, tested and Approved.

9. **Equipment Ratings:**

Electrical equipment for use indoor unclassified or Ordinary locations.

Certificate issued by:

J.E. Marquedant
VP, Manager - Electrical Systems

2 April 2020

Date

To verify the availability of the Approved product, please refer to www.approvalguide.com

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC. 1151 Boston-Providence Turnpike, Norwood, MA 02062 USA
T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmapprovals.com www.fmapprovals.com

SCHEDULE



to US Certificate Of Conformity No: FM16NUS0017

10. Description of Equipment:

The P1 sample gas pumps carry gases from various processes to analyzers. The gas circuit typically has additional analysis components such as sample gas probe, filter, flow meter, cooler, etc. The sample gas pump P1 consists of the main components, the pump head and motor. An eccentric converts the rotation of the motor into an up and down motion using a connecting rod, thus producing the pump mechanism. Inside the so-called pump body, above the bellows, which facilitates the pump motion, are inlet and outlet valves. The user connects the gas circuits to the sample gas pump through screw-in connections.

The P1 sample gas pumps are available as 12Vdc, 24Vdc, 115Vac, 60Hz or 230Vac, 50Hz. The 115Vac and 230Vac sample gas pumps have internal self resetting thermal protection built into the motor. The P1.1 sample gas pump is for general purpose non-hazardous locations.

Model Code Structure:

4228abc1def00FM. P1.1 Sample Gas Pump.

a = Motor voltage: 1, 2, 3 or 4.

b = Pump head position: 1 or 2.

c = Pump head material: 1, 2, 3 or 4.

d = Screw-in connections / pipe fitting: 0, 1, 2, 3, 5 or 6.

e = Mounting accessories: 0, 1 or 2.

f = Housing: 0 or 1

11. Test and Assessment Procedure and Conditions:

This Certificate has been issued in accordance with FM Approvals US Certification Requirements.

12. Schedule Drawings

A copy of the technical documentation has been kept by FM Approvals.

13. Certificate History

Details of the supplements to this certificate are described below:

Date	Description
11 th April 2016	Original Issue.
9 th December 2016	<u>Supplement 1:</u> Report Reference: – RR207245 dated 9 th December 2016. Description of the Change: Changes per this revision request are for the NI version of the product and don't affect this certificate. This certificate has been put into the new format.
2 nd April 2020	<u>Supplement 2:</u> Report Reference: – PR455937 dated 2 nd April 2020

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC. 1151 Boston-Providence Turnpike, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmaprovals.com www.fmaprovals.com

SCHEDULE



to US Certificate Of Conformity No: FM16NUS0017

Date	Description
	Description of the Change: Add option for gas pump cover DC motors.

FM Approvals

FM Approvals

FM Approvals

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC. 1151 Boston-Providence Turnpike, Norwood, MA 02062 USA
T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmaprovals.com www.fmaprovals.com

RMA-Formular und Erklärung über Dekontaminierung

Formulaire RMA et déclaration de décontamination



RMA-Nr./ Numéro de renvoi

Die RMA-Nr. bekommen Sie von Ihrem Ansprechpartner im Vertrieb oder Service. Bei Rücksendung eines Altgeräts zur Entsorgung tragen Sie bitte in das Feld der RMA-Nr. "WEEE" ein./ Le numéro d'autorisation de retour (RMA) est mis à votre disposition par votre interlocuteur à la vente ou au service. Lors du renvoi d'un appareil usagé en vue de sa mise au rebut, veuillez saisir "WEEE" dans le champ du n° RMA.

Zu diesem Rücksendeschein gehört eine Dekontaminierungserklärung. Die gesetzlichen Vorschriften schreiben vor, dass Sie uns diese Dekontaminierungserklärung ausgefüllt und unterschrieben zurücksenden müssen. Bitte füllen Sie auch diese im Sinne der Gesundheit unserer Mitarbeiter vollständig aus./ Une déclaration de décontamination fait partie intégrante de ce bulletin de retour. Les prescriptions légales vous obligent à nous renvoyer cette déclaration de décontamination remplie et signée. Veuillez la remplir également complètement au sens de la santé de nos employés.

Firma/ Société

Firma/ Société

Straße/ Rue

PLZ, Ort/ CP, localité

Land/ Pays

Gerät/ Appareil

Anzahl/ Nombre

Auftragsnr./ Numéro de commande

Ansprechpartner/ Interlocuteur

Name/ Nom

Abt./ Dépt.

Tel./ Tél.

E-Mail

Serien-Nr./ N° de série

Artikel-Nr./ N° d'article

Grund der Rücksendung/ Motif du retour

- ☐ Kalibrierung/ Calibrage ☐ Modifikation/ Modification
☐ Reklamation/ Réclamation ☐ Reparatur/ Réparation
☐ Elektroaltgerät/ Appareil électrique usagé (WEEE)
☐ andere/ autre

bitte spezifizieren/ veuillez spécifier

Ist das Gerät möglicherweise kontaminiert?/ L'appareil a-t-il été utilisé ?

- ☐ Nein, da das Gerät nicht mit gesundheitsschädlichen Stoffen betrieben wurde./ Non, car l'appareil n'a pas été utilisé avec des substances dangereuses pour la santé.
☐ Nein, da das Gerät ordnungsgemäß gereinigt und dekontaminiert wurde./ Non, car l'appareil a été nettoyé et décontaminé en bonne et due forme.
☐ Ja, kontaminiert mit:/ Oui, contaminé avec:



☐
explosiv/
explosif



☐
entzündlich/
inflammable



☐
brandfördernd/
comburant



☐
komprimierte
Gase/
gaz comprimés



☐
ätzend/
corrosif



☐
giftig,
Lebensgefahr/
toxique, danger
de mort



☐
gesundheitsge-
fährdend/
dangereux pour
la santé



☐
gesund-
heitsschädlich/
nocif pour la
santé



☐
umweltge-
fährdend/
dangereux pour
l'environnement

Bitte Sicherheitsdatenblatt beilegen!./ Merci de joindre la fiche technique de sécurité

Das Gerät wurde gespült mit:/ L'appareil a été rincé avec:

Diese Erklärung wurde korrekt und vollständig ausgefüllt und von einer dazu befugten Person unterschrieben. Der Versand der (dekontaminierten) Geräte und Komponenten erfolgt gemäß den gesetzlichen Bestimmungen.

Falls die Ware nicht gereinigt, also kontaminiert bei uns eintrifft, muss die Firma Bühler sich vorbehalten, diese durch einen externen Dienstleister reinigen zu lassen und Ihnen dies in Rechnung zu stellen.

Firmenstempel/ Cachet de l'entreprise

Cette déclaration a été correctement complétée et signée par une personne autorisée. L'envoi des appareils et composants (décontaminés) se fait selon les conditions légales.

Si la marchandise nous est retournée sans avoir été nettoyée, donc toujours contaminée, la société Bühler se réserve le droit de faire nettoyer le produit par un prestataire externe et de vous envoyer la facture correspondante.

Datum/ Date

rechtsverbindliche Unterschrift/ Signature autorisée



Vermeiden von Veränderung und Beschädigung der einzusendenden Baugruppe

Die Analyse defekter Baugruppen ist ein wesentlicher Bestandteil der Qualitätssicherung der Firma Bühler Technologies GmbH. Um eine aussagekräftige Analyse zu gewährleisten muss die Ware möglichst unverändert untersucht werden. Es dürfen keine Veränderungen oder weitere Beschädigungen auftreten, die Ursachen verdecken oder eine Analyse unmöglich machen.

Umgang mit elektrostatisch sensiblen Baugruppen

Bei elektronischen Baugruppen kann es sich um elektrostatisch sensible Baugruppen handeln. Es ist darauf zu achten, diese Baugruppen ESD-gerecht zu behandeln. Nach Möglichkeit sollten die Baugruppen an einem ESD-gerechten Arbeitsplatz getauscht werden. Ist dies nicht möglich sollten ESD-gerechte Maßnahmen beim Austausch getroffen werden. Der Transport darf nur in ESD-gerechten Behältnissen durchgeführt werden. Die Verpackung der Baugruppen muss ESD-konform sein. Verwenden Sie nach Möglichkeit die Verpackung des Ersatzteils oder wählen Sie selber eine ESD-gerechte Verpackung.

Einbau von Ersatzteilen

Beachten Sie beim Einbau des Ersatzteils die gleichen Vorgaben wie oben beschrieben. Achten Sie auf die ordnungsgemäße Montage des Bauteils und aller Komponenten. Versetzen Sie vor der Inbetriebnahme die Verkabelung wieder in den ursprünglichen Zustand. Fragen Sie im Zweifel beim Hersteller nach weiteren Informationen.

Einsenden von Elektroaltgeräten zur Entsorgung

Wollen Sie ein von Bühler Technologies GmbH stammendes Elektroprodukt zur fachgerechten Entsorgung einsenden, dann tragen Sie bitte in das Feld der RMA-Nr. „WEEE“ ein. Legen Sie dem Altgerät die vollständig ausgefüllte Dekontaminierungserklärung für den Transport von außen sichtbar bei. Weitere Informationen zur Entsorgung von Elektroaltgeräten finden Sie auf der Webseite unseres Unternehmens.

Éviter la modification et la détérioration du module à expédier

L'analyse d'unités défectueuses est un élément essentiel de l'Assurance Qualité de la société Bühler Technologies GmbH. Pour garantir une analyse pertinente, la marchandise doit être si possible contrôlée en l'état. Aucune modification ne doit être réalisée ni autre dommage se produire car les causes pourraient alors être masquées ou toute analyse serait rendue impossible.

Manipulation des modules à sensibilité électrostatique

Dans le cas d'unités électroniques, il peut s'agir de composants sensibles aux charges électrostatiques. Les composants doivent être traités en respectant les directives en matière de décharges électrostatiques. Selon le cas, les composants devraient être remplacés à un poste de travail ESD. Si cela n'est pas possible, des mesures respectant les directives en matière de décharges électrostatiques devraient être prises lors du remplacement. Le transport ne doit être réalisé que dans des conditions respectant les directives en matière de décharges électrostatiques. Les emballages des composants doivent être en conformité avec les directives en matière de décharges électrostatiques. Utilisez selon le cas l'emballage de pièces de rechange ou choisissez vous-même un emballage en conformité avec les directives en matière de décharges électrostatiques.

Montage de pièces de rechange

Veillez lors de l'insertion d'une pièce de rechange à ce que les conditions décrites ci-dessus soient respectées. Veillez à ce que le montage du produit et de tous les composants soit fait de manière appropriée. Remettez tous les câbles dans leur état d'origine avant la mise en service du produit. En cas de doute, adressez-vous au fabricant du produit pour avoir plus d'informations.

Renvoi d'appareils électriques usagés en vue de leur mise au rebut

Si vous souhaitez expédier un produit électrique manufacturé par Bühler Technologies GmbH en vue de sa mise au rebut correcte, veuillez saisir "WEEE" dans le champ du n° RMA. Pour le transport, joignez à l'appareil usagé la déclaration de décontamination entièrement remplie et bien visible de l'extérieur. Vous trouverez davantage d'informations concernant la mise au rebut des appareils électriques usagés sur le site Internet de notre entreprise.

